

RESEARCH

Open Access



Early detection of myocardial ischemia in resting ECG: analysis by HHT

Chun-Lin Wang¹, Chiu-Chi Wei², Cheng-Ting Tsai^{3,4}, Ying-Hsiang Lee^{3,5,6}, Lawrence Yu-Min Liu^{5,10}, Kang-Ying Chen^{3,7}, Yu-Jen Lin^{4,8} and Po-Lin Lin^{9,10*}

*Correspondence:
berlin831@gmail.com

⁹ Division of Cardiology,
Department of Internal Medicine,
Hsinchu MacKay Memorial
Hospital, No. 690, Sec.2,
Guangfu Rd., East Dist., Hsinchu
City 30071, Taiwan, ROC
Full list of author information is
available at the end of the article

Abstract

Background: Exercise electrocardiography (ECG) is a noninvasive test aiming at producing ischemic changes. However, resting ECG cannot be adopted in diagnosing myocardial ischemia till ST-segment depressions. Therefore, this study aimed to detect myocardial energy defects in resting ECG using the Hilbert–Huang transformation (HHT) in patients with angina pectoris.

Methods: Electrocardiographic recordings of positive exercise ECG by performing coronary imaging test (n = 26) and negative exercise ECG (n = 47) were collected. Based on the coronary stenoses severity, patients were divided into three categories: normal, < 50%, and ≥ 50%. During the resting phase of the exercise ECG, all 10-s ECG signals are decomposed by HHT. The RT intensity index, composed of the power spectral density of the P, QRS, and T components, is used to estimate the myocardial energy defect.

Results: After analyzing the resting ECG using HHT, the RT intensity index was significantly higher in patients with positive exercise ECG (27.96%) than in those with negative exercise ECG (22.30%) (p < 0.001). In patients with positive exercise ECG, the RT intensity index was gradually increasing with the severity of coronary stenoses: 25.25% (normal, n = 4), 27.14% (stenoses < 50%, n = 14), and 30.75% (stenoses ≥ 50%, n = 8). The RT intensity index of different coronary stenoses was significantly higher in patients with negative exercise ECG, except for the normal coronary imaging test.

Conclusions: Patients with coronary stenoses had a higher RT index at the resting stage of exercise ECG. Resting ECG analyzed using HHT could be a method for the early detection of myocardial ischemia.

Keywords: Exercise electrocardiography, Hilbert–Huang transform, Power spectral density, Myocardial energy

Background

Cardiovascular diseases (CVDs), including coronary artery disease (CAD), are the leading cause of death globally with an unmet need on decreasing mortality [1, 2]. CAD is pathologically characterized by atherosclerotic plaque accumulation in the epicardial arteries, whether obstructive or non-obstructive. Electrocardiography (ECG) measures the myocardial electrical activity widely used to detect CAD [3–6]. CAD or myocardial



© The Author(s) 2023. **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated in a credit line to the data.

ischemia is usually diagnosed based on the detection of repolarization abnormalities of ECG signals, mainly during ST-segment depressions [7]. Pathological Q waves or left bundle branch block could be another indirect sign of CAD during resting ECG. If a patient has a high clinical likelihood of CAD without significant ischemia changes during resting ECG, an exercise ECG test is suitable for measuring the initial, middle, and post-ECG exercise while strengthening the heart's oxygen consumption [7]. As the patient's body works harder during the exercise ECG test, limitation of the coronary blood flow due to obstructive CAD may result in ischemia changes during ECG. However, exercise ECG has limited the power to confirm obstructive CAD [7]. Muscle contraction, baseline wander, and powerline interference will interfere with ECG signals during ECG analysis [8]. If CAD cannot be excluded by clinical assessment, using noninvasive coronary computed tomography is recommended to establish the diagnosis [7, 9].

Additional analysis of ECG signals could be another method to improve the accuracy of the ECG exercise test. Various methods have been used to extract ECG features to diagnose a clinical disease, including Hilbert–Huang transformation (HHT) [10], which applies nonlinear and nonstationary signals and is a relatively new method used in biomedical data analysis [10]. Statistical characteristics are extracted from instinct mode functions obtained by applying HHT to R–R intervals. HHT decomposes the original ECG signals through the empirical mode decomposition (EMD) for myocardial energy analysis [11], and has been extensively used in disease detection, including heart failure, atrial fibrillation and CAD [10]. The addition of HHT in patients with suspected CAD could enhance the accuracy; however, the difference in myocardial ischemia in different stages of the ECG exercise test was less discussed [7, 10, 11]. This study aimed to detect the level of myocardial energy defect in resting ECG and analyze the noninvasive HHT test to predict CAD.

Results

After excluding the positive exercise ECG without coronary imaging test, a total of 73 patients who underwent exercise ECG were enrolled in the study, consisting of 47 patients (male: 34 and female: 13) with negative ECG as a reference group. Based on the coronary stenoses severity, patients with positive ECG exercise ($n=26$; male: 16 and female: 10) were divided into three groups: normal ($n=4$), $<50\%$ ($n=14$), and $\geq 50\%$ ($n=8$) stenoses (Fig. 1).

Compared with the reference group of negative exercise ECG, the following analysis models were designed: model 1, positive exercise ECG ($n=26$); model 2, stenoses $<50\%$ ($n=18$) and $\geq 50\%$ ($n=8$) stenoses; and model 3, normal ($n=4$), $<50\%$ ($n=14$), and $\geq 50\%$ ($n=8$) stenoses. All resting-stage recordings of exercise ECG were analyzed using HHT, and the myocardial energy defect was estimated using the RT intensity index (Table 1, Additional files 3, 5, 6, 7, 8, 11, 12 and 13).

Model 1: Comparing the energy difference of resting exercise ECG energy between the positive and negative exercise groups, the RT intensity index of the positive exercise ECG group ($27.96\% \pm 6.14\%$) was significantly higher than that of the negative group ($22.30\% \pm 4.34\%$) ($p < 0.001$) (Fig. 2, Table 2 and Additional file 1).

Model 2: Based on the coronary stenoses severity, patients with positive exercise ECG ($n=26$) were divided into two groups: $<50\%$ ($N=18$) and $\geq 50\%$ ($N=8$) coronary

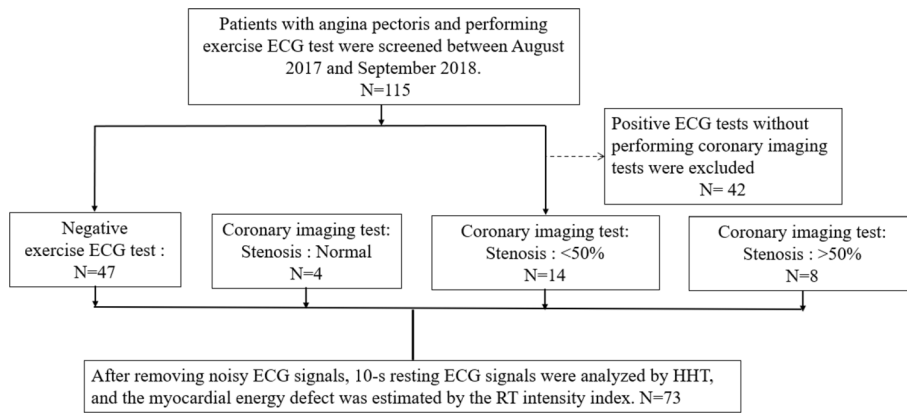


Fig. 1 Flow diagram of patient selection

Table 1 The severity distribution of patients between groups

Exercise ECG tests	Number	RT Index (%)	Std. error (%)	Upper bound (%)	Lower bound (%)
Negative	47	22.30	0.63	23.57	21.02
Positive					
Stenoses: 0%	4	25.25	2.95	34.65	15.85
Stenoses: < 50%	14	27.14	1.40	30.16	24.12
Stenoses: ≥ 50%	8	30.75	2.60	36.91	24.59

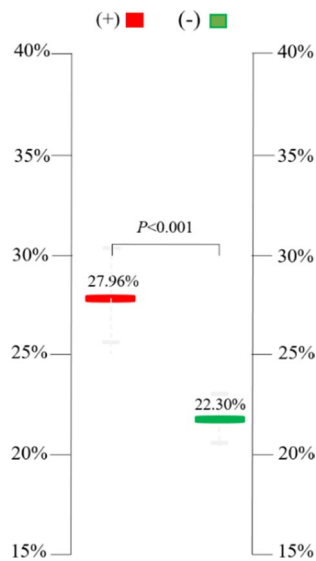


Fig. 2 The difference in myocardial electrical energy (RT index) between the positive and negative exercise ECG groups during the resting stage (Model 1)

stenoses (Fig. 3-A). The RT index of the group with < 50% (26.72% ± 5.27%) or ≥ 50% (30.75% ± 7.36%) coronary stenoses was significantly higher than that in the negative group (22.30% ± 4.34%) (p = 0.008 and p < 0.001) (Table 3, Additional file 2).

Table 2 The difference in RT index between negative and positive exercise ECG groups

Variable	Exercise ECG	Number	Male	Female	Age	RT index (%)	Std. deviation (%)	Std. error (%)	Upper bound (%)	Lower bound (%)	p-value
Threshold Model 1	Negative	47	34	13	50.68	22.30	4.34	0.63	23.57	21.02	<0.001
	Positive	26	16	10	49.38	27.96	6.14	1.20	30.44	25.48	

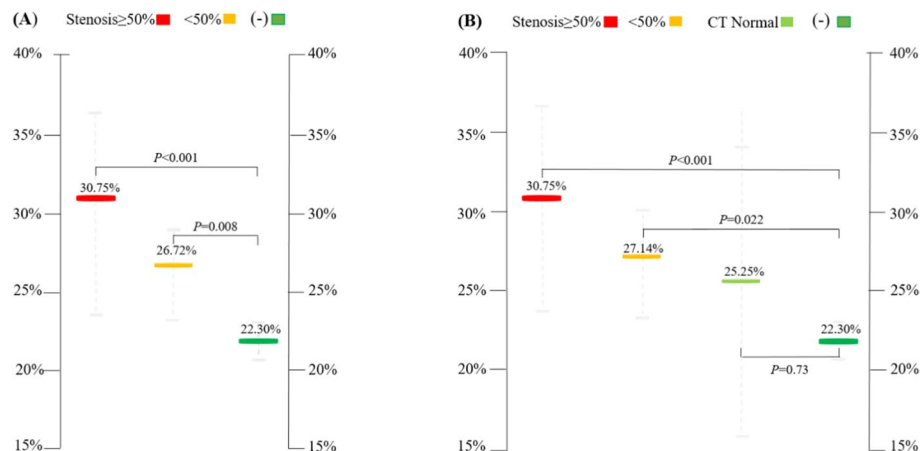


Fig. 3 The difference in myocardial electrical energy (RT index) between negative and positive exercise ECG groups with different coronary stenoses in the resting stage (**A**: model 2 and **B**: model 3, Additional files 4, 9, 10)

Model 3: Based on coronary stenoses severity, patients with positive exercise ECG ($n=26$) were divided into three groups: normal ($n=4$), $<50\%$ ($n=14$), and $\geq 50\%$ ($n=8$) stenoses $<50\%$ (Fig. 3-B). No significant difference in the RT index was observed between the negative exercise ECG ($22.30\% \pm 4.34\%$) and normal coronary image groups ($25.25\% \pm 5.91\%$; $p=0.73$). The RT index of coronary stenoses of $<50\%$ ($27.14\% \pm 5.23\%$) or $\geq 50\%$ ($30.75\% \pm 7.36\%$) was significantly higher ($p=0.022$ and $p<0.001$) (Table 3). The diagnostic accuracy of the RT index during the resting phase of the exercise ECG for differentiating between myocardial ischemia and different coronary stenoses, as quantified by the area under the receiver-operating characteristics curve (AUC) was 0.789 ($p<0.05$) (Fig. 4).

Discussion

The main findings of the present study indicated that patients with significant coronary stenoses had a higher RT index in the resting stage of exercise ECG. Moreover, resting ECG signals analyzed by HHT could be a method of the early detection of myocardial energy defects in patients with angina pectoris.

According to the 2019 European Society of Cardiology guidelines for the diagnosis and management of chronic coronary syndromes, a resting ECG is useful for the early detection of CAD [7, 12]. A resting ECG is an important tool for diagnosing myocardial ischemia, whereas dynamic ST-segment changes are recorded during ongoing angina or myocardial infarction. Although even ambulatory ECG monitoring is capable of detecting silent ischemia in chronic coronary syndrome patients, resting ECG cannot replace exercise ECG as it can rarely provide any information that could help in the diagnosis or prognosis of myocardial ischemia [7]. Therefore, an exercise ECG with increased myocardial oxygen consumption may be considered in patients with a clinical likelihood of CAD. However, exercise ECG has very limited diagnostic power in detecting obstructive CAD, compared with coronary imaging tests [7, 13]. Besides, a resting or exercise ECG with pre-existing repolarization abnormalities, such as pathological Q waves or conduction abnormalities, will influence the accuracy of detecting CAD. In an extensive study

Table 3 The difference in RT index based on different degrees of coronary stenoses

Variable	Exercise ECG	Number	Male	Female	Age	RT index (%)	Std. deviation (%)	Std. error (%)	Upper bound (%)	Lower bound (%)	p-value	
Threshold Model 1	Negative	47	34	13	50.68	22.30	4.34	0.63	23.57	21.02	<0.001	
	Positive	26	16	10	49.38	27.96	6.14	1.20	30.44	25.48		
Model 2	Coronary stenoses											
	< 50%	18	11	7	47.6	26.72	5.27	1.24	29.34	24.10	0.008	
Model 3	≥ 50%	8	5	3	53.38	30.75	7.36	2.60	36.91	24.59	<0.001	
	Normal	4	3	1	42.75	25.25	5.91	2.95	34.65	15.85	0.73	
	< 50%	14	8	6	49	27.14	5.23	1.40	30.16	24.12	0.022	
	≥ 50%	8	5	3	53.38	30.75	7.36	2.60	36.91	24.59	<0.001	

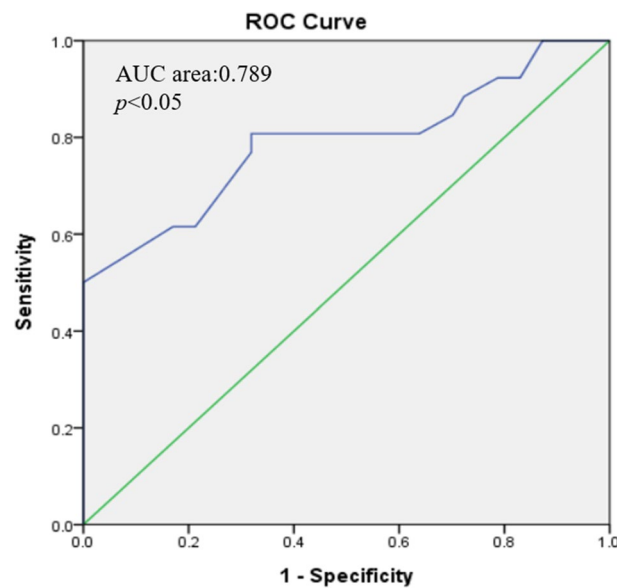


Fig. 4 Analysis of the receiver-operating (AUC) characteristics curve for differentiating between myocardial ischemia and different coronary stenoses using the RT index during the resting stage of the exercise ECG

of 3094 patients for >12 years (1969–1981), five elements (maximum exercise rhythm, number of exercises, CAD, angina pectoris type, age, and gender) had significant independent effects on exercise ECG testing sensitivity [14]. Exercise ECG combined with the functional image test could confirm the CAD diagnosis; however, the process is more time-consuming or costly [7].

The ECG reflects changes in the myocardial bioelectricity in the R^3 space in each cardiac cycle and presents the results in the R^2 space ECG. Muscle contraction, baseline wander, and powerline interference will interfere with ECG signals during analysis [8]. Various methods have been used to extract ECG feature disorders to diagnose a clinical disease, including wavelet analysis, discrete Fourier transform, EMD, second-order difference plot, wavelet packet decomposition, or HHT [2, 10, 12, 15–25]. The EMD has a large frequency distribution and high sample rate, especially in long time series [26], and is computationally expensive with some serious disadvantages such as border effects and mode mixing [27–30]. WT/FFT employs an integral method on a pre-established basis via the inner product method to determine the content of the base component in the data as a representative of the spectrum intensity, and the change of the disturbance frequency or wavelength may have occurred prior to the entire period of disturbance. The occurrence (the so-called intra-wave). HHT uses a differential method to decompose the signal into several IMFs with good symmetry properties. The perturbation frequency and amplitude of each IMF can change with time, and the manner of change is completely determined by the characteristics of the data itself. This basis is not pre-settled. Which is fixed and obtained by decomposing the signal itself through EMD, which belongs to the post-basis. The instantaneous frequency obtained by HHT has a clear physical meaning and can characterize the signal's local characteristics [31]. Despite the limited theoretical analysis, nonlinear and nonstationary signal problems can be solved with HHT [4, 5, 32, 33]. HHT

with EMD and Hilbert spectral analysis has been extensively used to analyze non-stationary signals, including heart failure, atrial fibrillation, and CAD [10]. Feature extraction of ECG signals using the HHT algorithm was independent of the 12-lead ECG detection method and had been widely used for detecting the myocardial energy defect [34, 35]. Patients with CAD could be distinguished from normal patients using features obtained by applying wavelet transformation and power spectral density for R–R intervals [10]. When comparing C1, C2, and C3 decomposed from pulse wave, no significant difference was observed in component C1 between healthy adults and patients with CAD but showed significant differences in component C3 ($p < 0.05$) [6]. Using the HHT algorithm in exercise ECG could improve the accuracy of diagnosis of myocardial ischemia [11]

In our previous study, we used two methods:

Method 1: Different stages exercise ECG before/during/post.

Method 2: Only use resting ECG before exercise.

The study reported that applying the HHT algorithm with the RT intensity and ST kinetic energy indices could reduce the pseudo-positive rate by 83.3%, as compared with exercise ECG only [11]. The ST kinetic energy index contained C4 and C5 components and is more sensitive to the QRS energy changes. Therefore, the ST kinetic energy index reflected a significant energy defect during the exercise stage of ECG [11]. However, a significant difference in the RT intensity index in the resting stage of exercise ECG was observed between patients with negative and positive exercise ECG [11]. In our study, we also found the myocardial energy defect in the resting stage of exercise ECG via the RT intensity index. In patients with positive exercise ECG, the RT intensity index was gradually increasing with the coronary stenoses severity. No significant difference in the RT intensity index was observed between positive exercise ECG with normal coronary imaging test and negative exercise ECG.

To the best of our knowledge, this was the first study to evaluate the relationship between coronary stenoses and myocardial energy difference of HHT in the resting stage of exercise ECG. Several study limitations should be considered in this study, i.e., the absence of prospective power and the small sample sizes. Therefore, we could not assess the benefits of detecting the early energy defect in the high-risk group based on future events. Further studies may investigate the accuracy, sensitivity, and specificity of the RT intensity index in predicting CAD during a resting ECG, as well as the effect of the differences between different ages and genders.

Conclusions

The resting stage of exercise ECG signal combined with HHT analysis can predict myocardial ischemia before the exercise stage. Patients with severe coronary stenoses had a higher RT index during the resting stage of exercise ECG than those with negative exercise ECG and normal or insignificant coronary stenoses. The resting ECG analyzed by HHT could be used as a new method for the early detection of myocardial ischemia before exercise ECG tests or invasive imaging studies.

Methods

Study population

In this retrospective study, all patients with angina pectoris and who underwent exercise ECG tests were screened between August 2017 and September 2018. The Institutional Review Board of Mackay Memorial Hospital approved this study protocol (IRB No. 17MMHIS004e), which waived the requirement for informed consent in this retrospective study. The treating physicians decided on the need to perform exercise ECG tests after excluding ECG abnormalities, including LBBB, paced rhythm, Wolff–Parkinson–White syndrome, ≥ 0.1 -mV ST-segment depression on resting ECG, or who are being treated with digitalis. The use of exercise ECG test was indicated by treating physicians and re-confirmed by other two cardiologists. Patients with positive exercise ECG were suggested to undergo coronary imaging, including coronary angiography or computed tomography. Based on the coronary stenoses severity, patients with positive exercise ECG were divided into three groups: normal, $< 50\%$, and $\geq 50\%$ stenoses. According to 2019 ESC Guidelines for the diagnosis and management of chronic coronary syndromes [7], the negative predictive value of exercise ECG was higher than positive predictive value. The likelihood of CAD was less than 15% if negative exercise ECG. Therefore, patients with negative exercise ECG were defined as a relative health group. Compared with patients with negative exercise ECG, analysis models were designed (model 1, positive exercise ECG; model 2, $< 50\%$ and $\geq 50\%$ stenoses; and model 3, normal, $< 50\%$, and $\geq 50\%$ stenoses).

Resting ECG signal data

After removing the baseline drift and the EMG signals in the first 7 s, stable resting ECG signals of 10 s were analyzed by pre-processing, feature extraction then classified by different coronary stenoses severities (Fig. 5).

The main ECG energy is concentrated at 0–40 Hz. The ECG signal can be divided into three components: P, QRS, and T based on waveform characteristics. In this

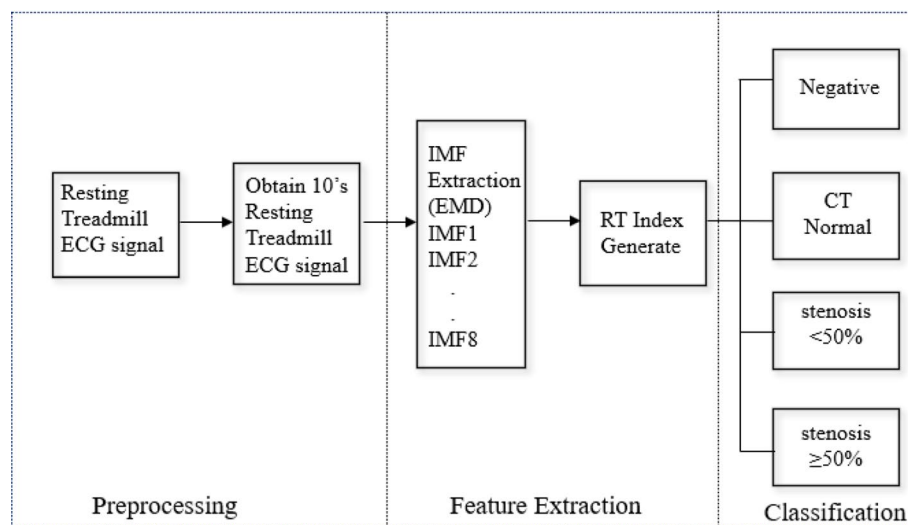


Fig. 5 Structure of proposed diagnostic blocks

study, the total ECG energy was decomposed into C1–8 spectrum components through EMD (Fig. 6):

- C1 and C2 are the highest frequency decomposition components of the QRS wave.
- C3 adds the P wave's decomposition components.
- C4 adds the decomposition component of the T wave, resulting from the superposition of three components: P, QRS, and T wave.
- C5 is a superposition of low-frequency components of P, QRS, and T waves.
- C6 represents the cardiac cycle, showing the heartbeat rhythm.
- C7 and C8 are cardiac physiological adjustment rhythms on a long-term scale, representing the heart's long-term rhythm.

C1, C2, ... to Cn represent disturbances from small to large wavelength scales. We can imagine the superposition of these disturbances as a small wave riding on an enormous wave, with still smaller waves on top of each of these small waves. The wavelength, frequency, and amplitude of each wave will change with time. Unlike the base assumed by FFT, the frequency and amplitude are unchanged and constant.

The RT intensity index was defined as:

$$RT = \frac{\alpha C1 + \beta C2 + \gamma C3}{\sum_{i=1}^8 C_i}$$

$\alpha|C1| + \beta|C2| + \gamma|C3|/|C \text{ total}|$ $\alpha/\beta/\gamma$ are weighting parameters of empirical correlation following rules

- (1) $(\alpha + \beta + \gamma)$ is less than 1.
- (2) $\alpha \geq \beta \geq \gamma$.

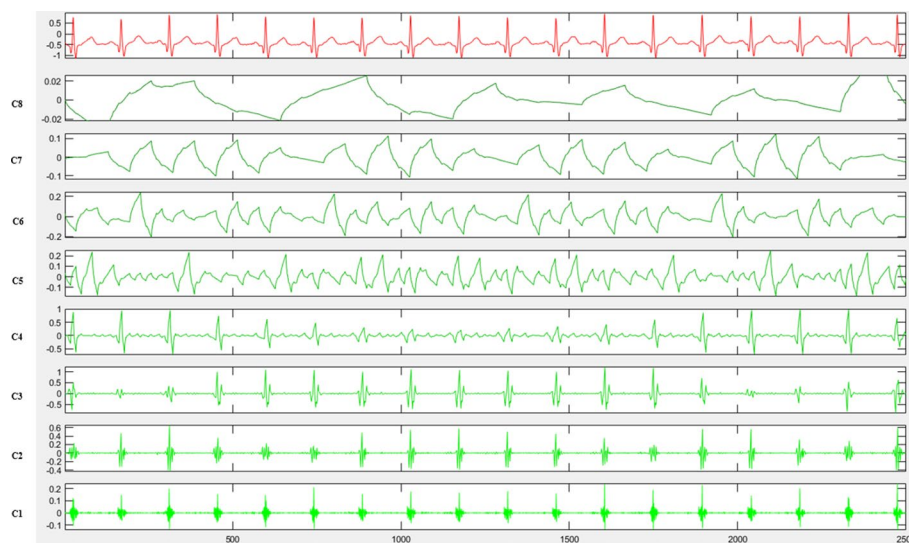


Fig. 6 A stable resting ECG signal with a sampling rate of 250 HZ in 10-s cycles is obtained in patients with negative exercise ECG

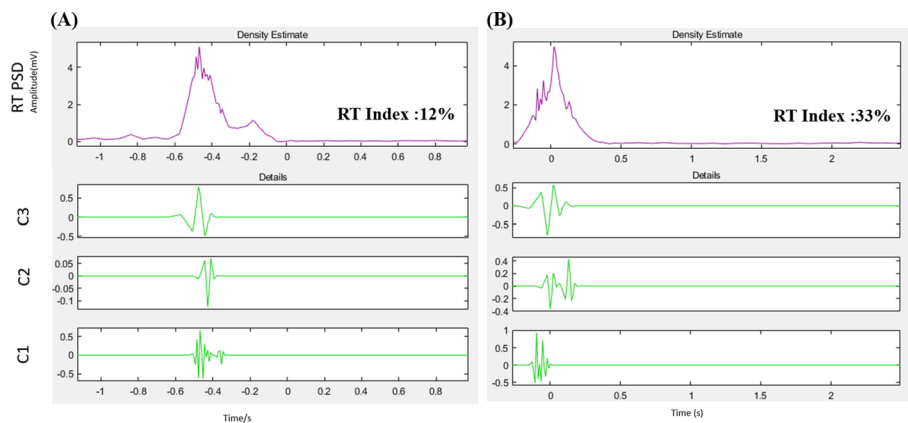


Fig. 7 The 10-s resting ECG signals were analyzed by the RT intensity index in patients with **A** negative exercise ECG and with **B** positive exercise ECG with coronary stenoses

the R wave intensity ratio (C1, C2, and C3 components compared to the total of C1–8) [11]. The RT index can display myocardial energy changes during resting ECG and is more sensitive in the QRS complex. All resting-stage electrocardiographic recordings of exercise ECG were analyzed using the RT intensity index (Fig. 7).

Statistical analysis

A two-way analysis of variance for repeated measures followed by a Bonferroni post-hoc test was used to analyze the RT index of resting-stage exercise ECG. The RT intensity index of negative exercise ECG was defined as a negative threshold. RT intensity indices of patients with positive exercise ECG were divided into three models based on the coronary stenoses severity. Compared with the negative threshold of the RT index, these models were used to analyze the positive exercise ECG group. Statistical significance was set at $p < 0.05$. All data analyses were performed using IBM SPSS statistics 20 for windows (IBM Corp., Chicago, IL, USA).

Abbreviations

CAD	Coronary artery disease
CVDs	Cardiovascular disease
ECG	Electrocardiography
EMD	Empirical mode decomposition
HHT	Hilbert–Huang transformation

Supplementary Information

The online version contains supplementary material available at <https://doi.org/10.1186/s12938-023-01089-9>.

- Additional file 1.** CT \geq 50% * 8.docx
- Additional file 2.** CT \geq 50% * 8.xlsx
- Additional file 3.** CT < 50% *14.docx
- Additional file 4.** CT < 50% *14.xlsx
- Additional file 5.** CT Normal * 4.docx
- Additional file 6.** CT Normal * 4.xlsx
- Additional file 7.** model 1 RT ANOVA.spv
- Additional file 8.** model 2 RT ANOVA.spv
- Additional file 9.** model 3 RT ANOVA.spv

Additional file 10. Negative * 47.docx

Additional file 11. Negative * 47.xlsx

Additional file 12. RT ANOVA.sav

Additional file 13. RT Intensity Index.xlsx

Acknowledgements

The authors would like to acknowledge the Cardio-Biomarker laboratory established by Dr. Kang-Ying Chen for the methodology and technical support on transferring ECG data to meaningful indices.

Author contributions

PLL, YHL, LYML, and KYC conceived and designed the study; CLW, CTT and YJL conducted the experiments and analyzed the data; PLL, KYC, CLW, and CCW interpreted the experiments results; CLW and PLL drafted and revised the manuscript. All authors read and approved the final manuscript.

Funding

This study did not receive any specific grants from funding agencies in the public, commercial, or not-for-profit sectors.

Availability of data and materials

Datasets used and/or analyzed during the current study are available from the corresponding author upon reasonable request.

Declarations

Ethics approval and consent to participate

This article does not contain any data or other information from studies or experimentation with human or animal patients.

Consent for publication

All authors consented to publication.

Competing interests

The authors declare that they have no competing interests.

Author details

¹Ph.D. Program of Technology Management, Chung Hua University, Hsinchu 30012, Taiwan, ROC. ²Department of Industrial Management, Chung Hua University, Hsinchu 30012, Taiwan, ROC. ³Cardiovascular Center, MacKay Memorial Hospital, No. 92, Sec. 2, Zhongshan N. Rd., Zhongshan Dist., Taipei City 104217, Taiwan, ROC. ⁴Department of Cosmetic Applications and Management, MacKay Junior College of Medicine, Nursing, and Management, Taipei City 112021, Taiwan, ROC. ⁵Department of Medicine, MacKay Medical College, No. 46, Sec. 3, Zhongzheng Rd., Sanzhi Dist., New Taipei City 252005, Taiwan, ROC. ⁶Department of Artificial Intelligence and Medical Application, MacKay Junior College of Medicine, Nursing, and Management, No. 46, Sec. 3, Zhongzheng Rd., Sanzhi Dist., New Taipei City 252005, Taiwan, ROC. ⁷Taoyuan Metro Corporation, Taoyuan City 337601, Taiwan, ROC. ⁸Big Light Optics Co., Ltd, Zhubei City, Hsinchu 302051, Taiwan, ROC. ⁹Division of Cardiology, Department of Internal Medicine, Hsinchu MacKay Memorial Hospital, No. 690, Sec.2, Guangfu Rd., East Dist., Hsinchu City 30071, Taiwan, ROC. ¹⁰Department of Nursing, MacKay Junior College of Medicine, Nursing, and Management, No. 92, Shengjing Rd., Beitou Dist., Taipei City 112021, Taiwan, ROC.

Received: 6 August 2022 Accepted: 1 March 2023

Published online: 10 March 2023

References

1. Roth GA, Mensah GA, Johnson CO, Addolorato G, Ammirati E, Baddour LM, Barengo NC, Beaton AZ, Benjamin EJ, Benziger CP, et al. Global burden of cardiovascular diseases and risk factors, 1990–2019: update from the GBD 2019 study. *J Am Coll Cardiol.* 2020;76(25):2982–3021. <https://doi.org/10.1016/j.jacc.2020.11.010>.
2. Gupta V, Mittal M, Mittal V. An efficient low computational cost method of R-peak detection. *Wirel Pers Commun.* 2021;118(1):359–81. <https://doi.org/10.1007/s11277-020-08017-3>.
3. Lenka B. Time-frequency analysis of non-stationary electrocardiogram signals using Hilbert-Huang Transform. In: 2015 International conference on communications and signal processing (ICCSPP). IEEE; 2015. pp. 1156–9. <https://doi.org/10.1109/ICCSPP.2015.7322686>.
4. Tarasiuk T, Zunino Y, Bueno-Lopez M, Silvestro F, Pilatis A, Molinas M. Frequency fluctuations in marine microgrids: origins and identification tools. *IEEE Electrific Mag.* 2020;8(3):40–6. <https://doi.org/10.1109/MELE.2020.3005698>.
5. Adnan NF, Ghazali MF, Amin MM, Hamat AMA. Leak detection in gas pipeline by acoustic and signal processing—a review. *Mater Sci Eng.* 2015;100:012013. <https://doi.org/10.1088/1757-899X/100/1/012013>.

6. Li FF, Sun R, Xue S, Qian P, Yan HX, Zhang WF, Sun ZM, Zhang HK, Wang YQ. Pulse signal analysis of patients with coronary heart diseases using Hilbert-Huang transformation and time-domain method. *Chin J Integr Med*. 2015;21(5):355–60. <https://doi.org/10.1007/s11655-015-2173-7>.
7. Knuuti J, Wijns W, Saraste A, Capodanno D, Barbato E, Funck-Brentano C, Prescott E, Storey RF, Deaton C, Cuisset T, et al. 2019 ESC guidelines for the diagnosis and management of chronic coronary syndromes. *Eur Heart J*. 2020;41(3):407–77. <https://doi.org/10.1093/eurheartj/ehz425>.
8. Karagiannis A, Constantinou P. Noise-assisted data processing with empirical mode decomposition in biomedical signals. *IEEE Trans Inf Technol Biomed*. 2011;15(1):11–8. <https://doi.org/10.1109/TITB.2010.2091648>.
9. Gupta V, Rathore NS, Arora AK, Gupta S, Kanungo A, Salim NA, Gupta NK. Electrocardiogram signal pattern recognition using PCA and ICA on different databases for improved health management. *Int J Appl Pattern Recogn*. 2022;7(1):41–63. <https://doi.org/10.1504/IJAPR.2022.122273>.
10. Altan G, Kutlu Y, Allahverdi N. A new approach to early diagnosis of congestive heart failure disease by using Hilbert-Huang transform. *Comput Methods Programs Biomed*. 2016;137:23–34. <https://doi.org/10.1016/j.cmpb.2016.09.003>.
11. Lin P-L, Chen K-Y, Ma H, Wang C-L, Lin YJ. Preliminary study a non-invasion method on early cardiac energy defect based on Hilbert Huang Transform. *Med Hypotheses*. 2020;144:110205. <https://doi.org/10.1016/j.mehy.2020.110205>.
12. Gupta V, Mittal M. R-peak detection for improved analysis in health informatics. *Int J Med Eng Inf*. 2021;13(3):213–23. <https://doi.org/10.1504/IJMEI.2021.114888>.
13. Knuuti J, Ballo H, Juarez-Orozco LE, Saraste A, Kolh P, Rutjes AWS, Juni P, Windecker S, Bax JJ, Wijns W. The performance of non-invasive tests to rule-in and rule-out significant coronary artery stenoses in patients with stable angina: a meta-analysis focused on post-test disease probability. *Eur Heart J*. 2018;39(35):3322–30. <https://doi.org/10.1093/eurheartj/ehy267>.
14. Guthrie RB, Vlodaver Z, Nicoloff DM, Edwards J. Pathology of stable and unstable angina pectoris. *Circulation*. 1975;51(6):1059–63. <https://doi.org/10.1161/01.CIR.51.6.1059>.
15. Gupta V, Mittal M, Mittal V, Saxena NK. A critical review of feature extraction techniques for ECG signal analysis. *J Inst Engineers (India): Ser B*. 2021;102(5):1049–60. <https://doi.org/10.1007/s40031-021-00606-5>.
16. Gupta V, Mittal M, Mittal V, Saxena NK. BP signal analysis using emerging techniques and its validation using ECG signal. *Sens Imaging*. 2021;22(1):25. <https://doi.org/10.1007/s11220-021-00349-z>.
17. Gupta V, Mittal M, Mittal V, Gupta A. An efficient AR modelling-based electrocardiogram signal analysis for health informatics. *Int J Med Eng Inf*. 2022;14(1):74–89. <https://doi.org/10.1504/IJMEI.2022.119314>.
18. Gupta V, Mittal M, Mittal V, Sharma AK, Saxena NK. A novel feature extraction-based ECG signal analysis. *J Inst Engineers (India): Ser B*. 2021;102(5):903–13. <https://doi.org/10.1007/s40031-021-00591-9>.
19. Gupta V, Mittal M, Mittal V, Chaturvedi Y. Detection of R-peaks using fractional Fourier transform and principal component analysis. *J Ambient Intell Humaniz Comput*. 2022;13(2):961–72. <https://doi.org/10.1007/s12652-021-03484-3>.
20. Gupta V, Mittal M, Mittal V. A Novel FrWT based arrhythmia detection in ECG signal using YWARA and PCA. *Wireless Pers Commun*. 2022;124(2):1229–46. <https://doi.org/10.1007/s11277-021-09403-1>.
21. Gupta V, Mittal M, Mittal V. FrWT-PPCA-based R-peak detection for improved management of healthcare system. *IETE J Res*. 2021. <https://doi.org/10.1080/03772063.2021.1982412>.
22. Gupta V, Saxena NK, Kanungo A, Gupta A, Kumar P. A review of different ECG classification/detection techniques for improved medical applications. *Int J Syst Assur Eng Manag*. 2022. <https://doi.org/10.1007/s13198-021-01548-3>.
23. Gupta V, Saxena NK, Kanungo A, Kumar P, Diwania S. PCA as an effective tool for the detection of R-peaks in an ECG signal processing. *Int J Syst Assur Eng Manag*. 2022. <https://doi.org/10.1007/s13198-022-01650-0>.
24. Balasubramanian K, Ananthamoorthy NP. Robust retinal blood vessel segmentation using convolutional neural network and support vector machine. *J Ambient Intell Humaniz Comput*. 2021;12(3):3559–69. <https://doi.org/10.1007/s12652-019-01559-w>.
25. Gupta V, Mittal M, Mittal V. R-peak detection using chaos analysis in standard and real time ECG databases. *IRBM*. 2019;40(6):341–54. <https://doi.org/10.1016/j.irbm.2019.10.001>.
26. Bowman DC, Lees JM. The Hilbert-Huang transform: a high resolution spectral method for nonlinear and non-stationary time series. *Seismol Res Lett*. 2013;84(6):1074–80. <https://doi.org/10.1785/0220130025>.
27. Liu Z, Bai W, Chen G. A new short-term load forecasting model of power system based on HHT and ANN. In: Proceedings of the 7th international conference on Advances in Neural Networks 2010, vol. 2. pp. 448–54. https://doi.org/10.1007/978-3-642-13318-3_56.
28. Wang T, Zhang M, Yu Q, Zhang H. Comparing the applications of EMD and EEMD on time–frequency analysis of seismic signal. *J Appl Geophys*. 2012;83:29–34. <https://doi.org/10.1016/j.jappgeo.2012.05.002>.
29. Huang Y, Di H, Malekian R, Qi X, Li Z. Noncontact measurement and detection of instantaneous seismic attributes based on complementary ensemble empirical mode decomposition. *Energies*. 2017;10(10):1655. <https://doi.org/10.3390/en10101655>.
30. Shen W-C, Chen Y-H, Wu A-Y. Low-complexity sinusoidal-assisted EMD (SAEMD) algorithms for solving mode-mixing problems in HHT. *Digit Signal Process*. 2014;24:170–86. <https://doi.org/10.1016/j.dsp.2013.08.004>.
31. Li X-l, Chen S-j, Liu S-m, Li Z-h. AE waveform characteristics of rock mass under uniaxial loading based on Hilbert–Huang transform. *J Cent South Univ*. 2021;28(6):1843–56. <https://doi.org/10.1007/s11771-021-4734-6>.
32. Sun X, Zhou L, Chang S, Liu Z. Using CNN and HHT to predict blood pressure level based on photoplethysmography and its derivatives. *Biosensors (Basel)*. 2021;11(4):120. <https://doi.org/10.3390/bios11040120>.

33. Mohammed AA, Haris SM. Using energy time-frequency of Hilbert Huang transform to analyze the performance of the variable valve timing engine. *Sci Rep.* 2022;12(1):2382. <https://doi.org/10.1038/s41598-022-06404-3>.
34. García S, Romo M, Alcántara LJSD, Engineering E. Analysis of non-linear and non-stationary seismic recordings of Mexico city. *Soil Dynam Earthq Eng.* 2019;127:105859. <https://doi.org/10.1016/j.soildyn.2019.105859>.
35. Paithane A, Bormane D. Electrocardiogram signal analysis using empirical mode decomposition and Hilbert spectrum. In: 2015 International Conference on Pervasive Computing (ICPC). IEEE; 2015. pp. 1–4. <https://doi.org/10.1109/pervasive.2015.7087042>.

Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Ready to submit your research? Choose BMC and benefit from:

- fast, convenient online submission
- thorough peer review by experienced researchers in your field
- rapid publication on acceptance
- support for research data, including large and complex data types
- gold Open Access which fosters wider collaboration and increased citations
- maximum visibility for your research: over 100M website views per year

At BMC, research is always in progress.

Learn more biomedcentral.com/submissions

